


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 2 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130144
Name		CHRISTOPHER M. CHAPMAN	ID# 6390 Date 23 MAR 10
A	Agency	EDF4 ELMENDORF AFB	Phone # 552-0176
Instrument Location 8517 20TH STREET ELMENDORF AFB, AK 99506			
Alco S/N		X124658	Target Value .081 High Pressure 1200
B	Alco Test Value Average	.084	.083
		1st Alco	2nd Alco
Signature			
(OVER)			


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 5th day of April, 2010.

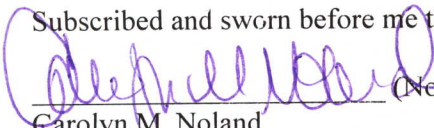  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130144 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130144

MARCH 23, 2010

OPERATOR'S NAME:  
CHAPMAN CHRISTOPHER M  
OPERATOR'S NUMBER: 6390  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
VOC

O.L. #: 1  
DEPT/AGENCY: EDF4  
CASE/REPORT:  
TEST TYPE: U  
ALCO TARGET VALUE: .001 ✓  
ALCO S/N: X124658 ✓

### — BREATH ANALYSIS —

.001 ADJUSTED FOR 29.70 in  
ALCO TARGET .000 09:09  
BLANK TEST .000 09:10  
INTERNAL STANDARD VERIFIED 09:10  
ALCO TU 29.70 in .004 ✓ 09:10  
BLANK TEST .000 09:11  
SUBJECT SAMPLE .000 09:11  
BLANK TEST .000 09:12  
ALCO TU 29.70 in .003 ✓ 09:13  
BLANK TEST .000 09:13

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130144 ✓

MARCH 23, 2010 ✓  
TIME 09:07

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 50c  
BREATH TUBE: 42c  
BAROMETER: 29.72 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHI  
JKLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~